



CERTIFICATE OF ANALYSIS

Issued by an ISO/IEC 17025-accredited laboratory · raw data appended (page 2)

PASS

QC released for dispatch



Scan to verify

Adamax — 10mg

Pro-Gly-Pro-Glu-OH (ACTH 4-10 analogue, acetylated / amidated)

1. PRODUCT IDENTIFICATION

Synonym	Pro-Gly-Pro-Glu-OH (ACTH 4-10 analogue, acetylated / amidated)	Label claim	10mg
Sequence / structure	—	Lot / Batch	ZX261008-254 / B70564
Mol. formula	C56H84N14O14S	Manufacture date	8 Oct 2026
Mol. weight	1217.42 g/mol	Date of analysis	9 Oct 2026
CAS number	2642232-10-6	Storage	-20 °C, dark, desiccated
Salt form	Acetate salt		

2. ANALYTICAL TEST RESULTS

Test	Method	Specification	Result	Verdict
Appearance	Visual	White/off-white powder	White to off-white lyophilized powder	PASS
Identity (ESI-MS)	LC-MS	Matches 1217.42 Da	1217.42 Da (Δ 0 ppm)	PASS
Purity	RP-HPLC, UV 220 nm	$\geq 98.0\%$ area	98.34%	PASS
Related substances	RP-HPLC	Single ≤ 1.0 / Total $\leq 2.0\%$	0.77 / 1.66%	PASS
Water content	Karl Fischer (USP <921>)	$\leq 8.0\%$	1.8%	PASS
Counter-ion: acetate	Ion chromatography	Report (3.0–15.0%)	5.2%	PASS
Net peptide content	Amino-acid analysis	$\geq 80.0\%$	90.9%	PASS
Bacterial endotoxin	LAL kinetic (USP <85>)	< 5.0 EU/mg	0.15 EU/mg	PASS
Heavy metals	ICP-MS (ICH Q3D)	Conforms	Conforms	PASS

CONCLUSION

All tested parameters CONFORM to the acceptance specifications. The batch is of high chromatographic purity ($\geq 98\%$) with an impurity profile, identity and residual/contaminant results meeting pharmaceutical-grade quality requirements. Material released. Supporting RP-HPLC chromatogram and ESI-MS spectrum are appended on page 2.

DLW.

Dr. Li Wenhua

Analyst · 9 Oct 2026 · Zhongxi Research Institute

DFH.

Dr. Fang Hong (QC Manager)

Approved by · 9 Oct 2026 · Zhongxi Research Institute




APPENDIX — ANALYTICAL RAW DATA

Adamax 10mg · Lot ZX261008-254 · Cert. ZXR-COA-2026-34249




Scan to verify

Figure 1. RP-HPLC Chromatogram (UV 220 nm)

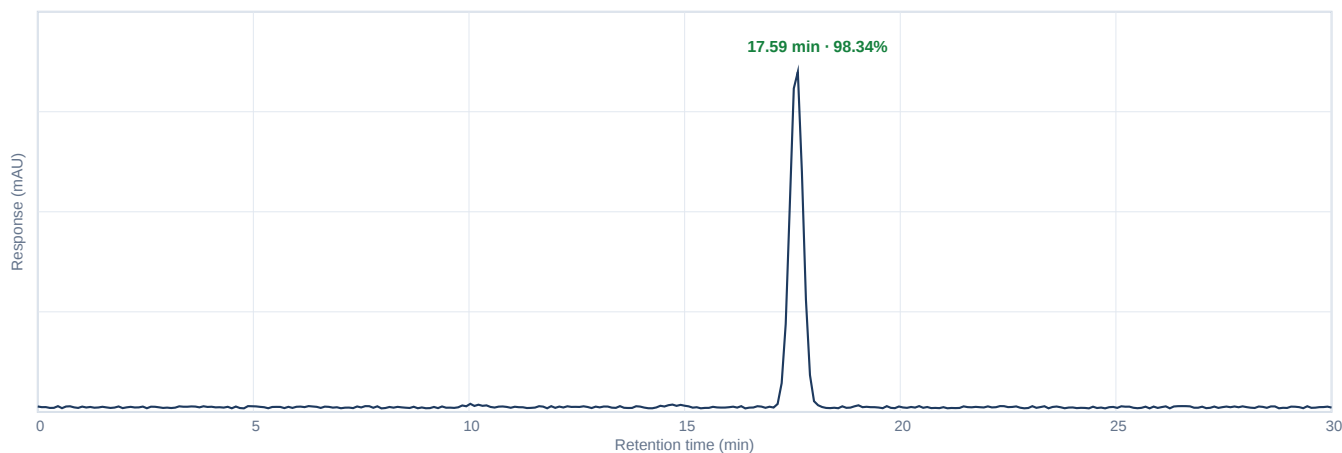

Peak #	RT (min)	Area (μV·s)	Area %	Assignment
1	17.59	1080638	98.34	Main (target)
2	10.08	6940	0.71	Impurity / related substance
3	14.84	5684	0.61	Impurity / related substance
4	19.02	3129	0.29	Impurity / related substance
5	23.65	505	0.05	Impurity / related substance

Figure 2. ESI-MS Spectrum (positive ion mode)

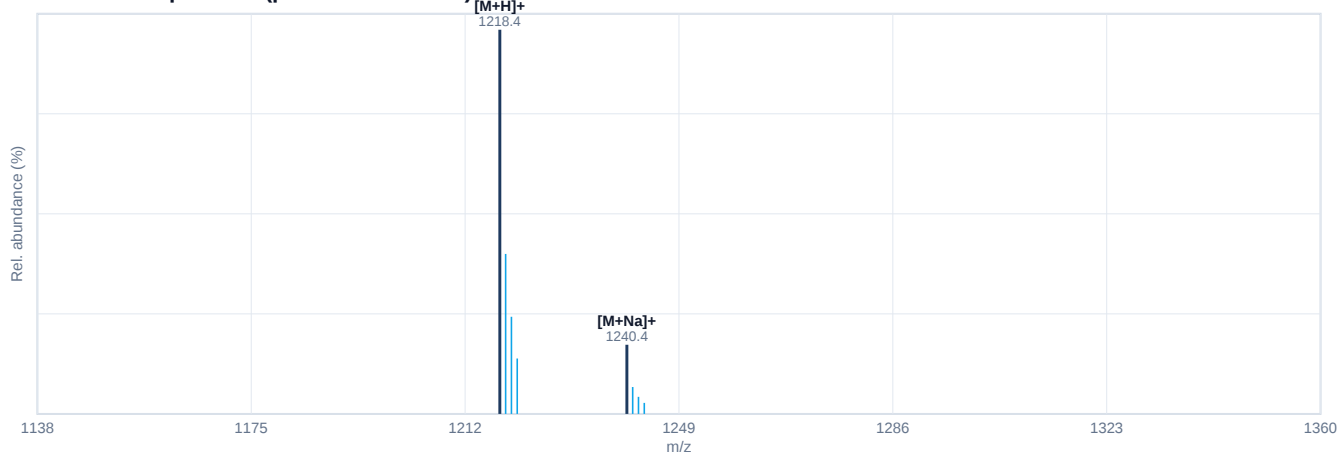

Interpretation

Identity confirmed by ESI-MS. Observed ions [M+H]⁺ 1218.4, [M+Na]⁺ 1240.4 deconvolute to a neutral monoisotopic-average mass of 1217.42 Da (theoretical 1217.42 Da; mass error 0 ppm), consistent with Adamax. No co-eluting species above 0.5% indicative of misidentification.

Methods — RP-HPLC: Agilent 1260 Infinity II; Zorbax SB-C18 4.6×250 mm, 5 μm; A: 0.1% TFA in water, B: 0.1% TFA in MeCN; 10–70% B over 30 min; 1.0 mL/min; 25 °C; 20 μL injection. MS: AB Sciex TripleTOF, ESI⁺, capillary 4.5 kV, deconvolution by Bio Tool Kit. KF: Metrohm 901. IC: Thermo Dionex ICS-6000. ICP-MS: Agilent 7900.