



CERTIFICATE OF ANALYSIS

Issued by an ISO/IEC 17025-accredited laboratory · raw data appended (page 2)

PASS

QC released for dispatch



Scan to verify

Glutathione — 600mg

Reduced Glutathione

1. PRODUCT IDENTIFICATION

Synonym	Reduced Glutathione	Label claim	600mg
Sequence / structure	—	Lot / Batch	ZX260512-956 / B31965
Mol. formula	C10H17N3O6S	Manufacture date	13 May 2026
Mol. weight	307.32 g/mol	Date of analysis	23 May 2026
CAS number	70-18-8	Storage	-20 °C, dark, desiccated
Salt form	Free base / N/A		

2. ANALYTICAL TEST RESULTS

Test	Method	Specification	Result	Verdict
Appearance	Visual	Per monograph	White crystalline powder	PASS
Identity	LC-MS + ¹ H-NMR	Matches 307.32 Da & ref	307.32 Da; conforms	PASS
Assay / Purity	RP-HPLC	≥ 98.0%	98.36%	PASS
Related substances	RP-HPLC	Total ≤ 2.0%	1.64%	PASS
Water content	Karl Fischer	≤ 5.0%	4.3%	PASS
Residual solvents	GC head-space (ICH Q3C)	Conforms	Conforms	PASS
Heavy metals	ICP-MS (ICH Q3D)	Conforms	Conforms	PASS

CONCLUSION

All tested parameters CONFORM to the acceptance specifications. The batch is of high chromatographic purity (≥ 98%) with an impurity profile, identity and residual/contaminant results meeting pharmaceutical-grade quality requirements. Material released. Supporting RP-HPLC chromatogram and ESI-MS spectrum are appended on page 2.

DXP.

Dr. Xu Ping

Analyst · 23 May 2026 · Zhongxi Research Institute

DLX.

Dr. Lin Xia (QC Manager)

Approved by · 23 May 2026 · Zhongxi Research Institute




APPENDIX — ANALYTICAL RAW DATA

Glutathione 600mg · Lot ZX260512-956 · Cert. ZXR-COA-2026-84021




Scan to verify

Figure 1. RP-HPLC Chromatogram (UV 220 nm)

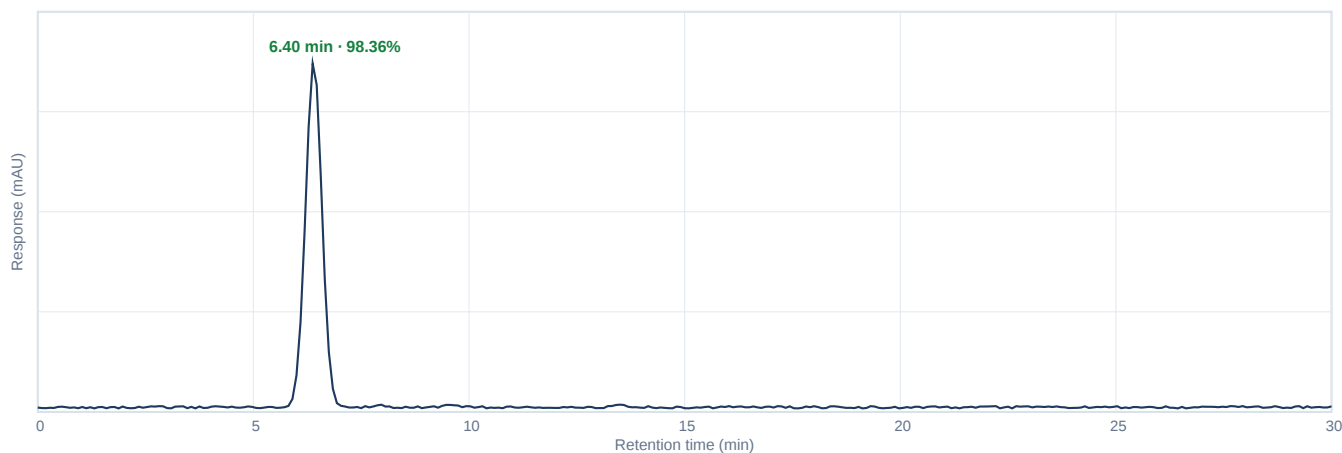

Peak #	RT (min)	Area (μV·s)	Area %	Assignment
1	6.40	945191	98.36	Main (target)
2	7.95	6190	0.62	Impurity / related substance
3	13.51	5566	0.51	Impurity / related substance
4	9.55	4551	0.46	Impurity / related substance
5	23.29	465	0.05	Impurity / related substance

Figure 2. ESI-MS Spectrum (positive ion mode)

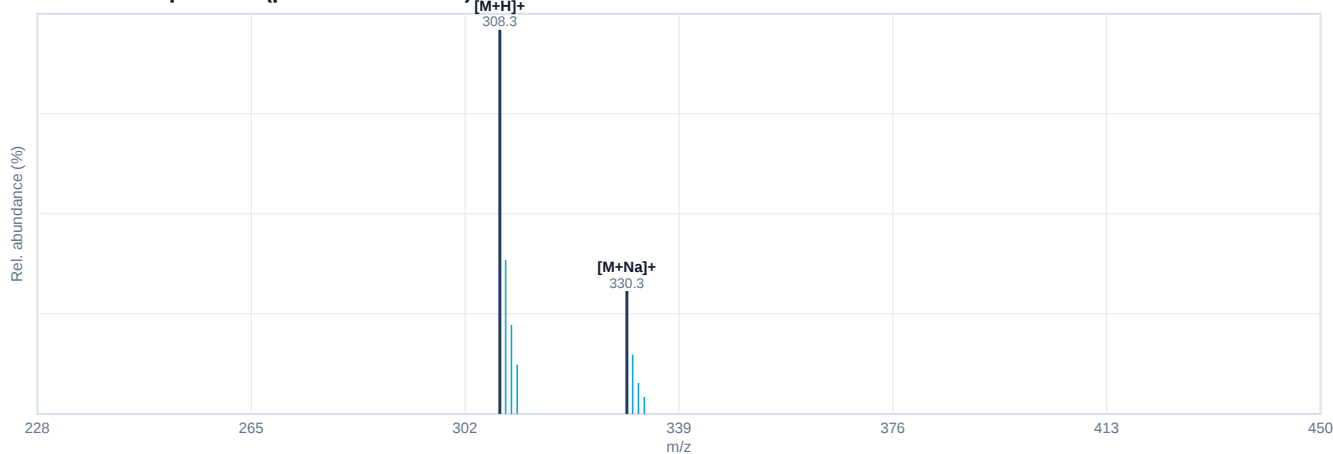

Interpretation

Identity confirmed by ESI-MS. Observed ions [M+H]⁺ 308.3, [M+Na]⁺ 330.3 deconvolute to a neutral monoisotopic-average mass of 307.32 Da (theoretical 307.32 Da; mass error 0 ppm), consistent with Glutathione. No co-eluting species above 0.5% indicative of misidentification.

Methods — RP-HPLC: Agilent 1260 Infinity II; Zorbax SB-C18 4.6×250 mm, 5 μm; A: 0.1% TFA in water, B: 0.1% TFA in MeCN; 10–70% B over 30 min; 1.0 mL/min; 25 °C; 20 μL injection. MS: AB Sciex TripleTOF, ESI⁺, capillary 4.5 kV, deconvolution by Bio Tool Kit. KF: Metrohm 901. IC: Thermo Dionex ICS-6000. ICP-MS: Agilent 7900.