



CERTIFICATE OF ANALYSIS

Issued by an ISO/IEC 17025-accredited laboratory · raw data appended (page 2)

PASS

QC released for dispatch



Scan to verify

Kisspeptin-10 — 5mg

Kisspeptin

1. PRODUCT IDENTIFICATION

Synonym	Kisspeptin	Label claim	5mg
Sequence / structure	Tyr-Asn-Trp-Asn-Ser-Phe-Gly-Leu-Arg-Phe-NH ₂	Lot / Batch	ZX260512-699 / B40441
Mol. formula	C ₆₃ H ₈₃ N ₁₇ O ₁₄	Manufacture date	29 May 2026
Mol. weight	1302.44 g/mol	Date of analysis	7 Jun 2026
CAS number	374675-21-5	Storage	-20 °C, dark, desiccated
Salt form	Acetate salt		

2. ANALYTICAL TEST RESULTS

Test	Method	Specification	Result	Verdict
Appearance	Visual	White/off-white powder	White to off-white lyophilized powder	PASS
Identity (ESI-MS)	LC-MS	Matches 1302.44 Da	1302.46 Da (Δ 15 ppm)	PASS
Purity	RP-HPLC, UV 220 nm	$\geq 98.0\%$ area	99.03%	PASS
Related substances	RP-HPLC	Single ≤ 1.0 / Total $\leq 2.0\%$	0.49 / 0.97%	PASS
Water content	Karl Fischer (USP <921>)	$\leq 8.0\%$	2.4%	PASS
Counter-ion: acetate	Ion chromatography	Report (3.0–15.0%)	11.0%	PASS
Net peptide content	Amino-acid analysis	$\geq 80.0\%$	85.2%	PASS
Bacterial endotoxin	LAL kinetic (USP <85>)	< 5.0 EU/mg	0.05 EU/mg	PASS
Heavy metals	ICP-MS (ICH Q3D)	Conforms	Conforms	PASS

CONCLUSION

All tested parameters CONFORM to the acceptance specifications. The batch is of high chromatographic purity ($\geq 98\%$) with an impurity profile, identity and residual/contaminant results meeting pharmaceutical-grade quality requirements. Material released. Supporting RP-HPLC chromatogram and ESI-MS spectrum are appended on page 2.

DZK.

Dr. Zhou Kai

Analyst · 7 Jun 2026 · Zhongxi Research Institute

DLX.

Dr. Lin Xia (QC Manager)

Approved by · 7 Jun 2026 · Zhongxi Research Institute




APPENDIX — ANALYTICAL RAW DATA

Kisspeptin-10 5mg · Lot ZX260512-699 · Cert. ZXR-COA-2026-25601




Scan to verify

Figure 1. RP-HPLC Chromatogram (UV 220 nm)

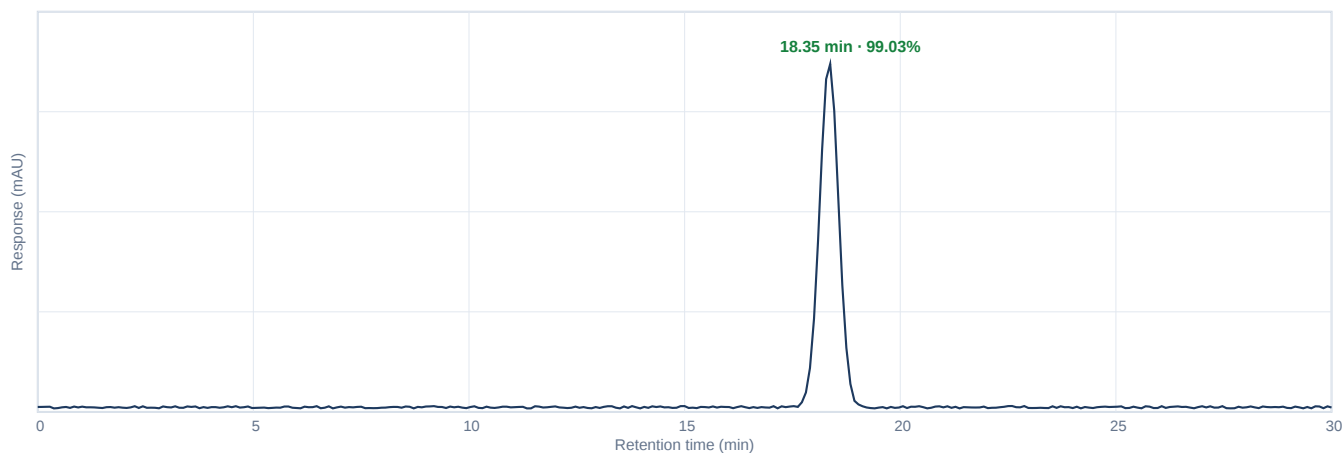

Peak #	RT (min)	Area (μV·s)	Area %	Assignment
1	18.35	1038885	99.03	Main (target)
2	22.53	5176	0.49	Impurity / related substance
3	23.49	364	0.04	Impurity / related substance

Figure 2. ESI-MS Spectrum (positive ion mode)

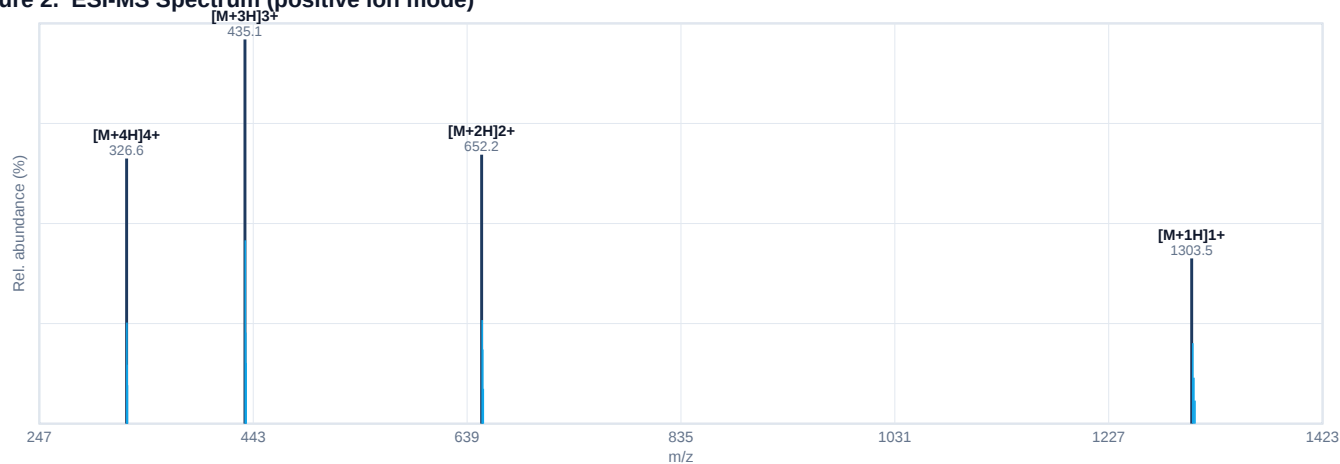

Interpretation

Identity confirmed by ESI-MS. Observed ions [M+1H]¹⁺ 1303.5, [M+2H]²⁺ 652.2, [M+3H]³⁺ 435.1, [M+4H]⁴⁺ 326.6 deconvolute to a neutral monoisotopic average mass of 1302.46 Da (theoretical 1302.44 Da; mass error 15 ppm), consistent with Kisspeptin-10. No co-eluting species above 0.5% indicative of misidentification.

Methods — RP-HPLC: Agilent 1260 Infinity II; Zorbax SB-C18 4.6×250 mm, 5 μm; A: 0.1% TFA in water, B: 0.1% TFA in MeCN; 10–70% B over 30 min; 1.0 mL/min; 25 °C; 20 μL injection. MS: AB Sciex TripleTOF, ESI+, capillary 4.5 kV, deconvolution by Bio Tool Kit. KF: Metrohm 901. IC: Thermo Dionex ICS-6000. ICP-MS: Agilent 7900.