



CERTIFICATE OF ANALYSIS

Issued by an ISO/IEC 17025-accredited laboratory · raw data appended (page 2)

PASS

QC released for dispatch



Scan to verify

N-Acetyl Semax Amideate — 10mg

N-Acetyl-(Met-Glu-His-Phe-Pro-Gly-Pro)-NH₂

1. PRODUCT IDENTIFICATION

Synonym	N-Acetyl-(Met-Glu-His-Phe-Pro-Gly-Pro)-NH ₂	Label claim	10mg
Sequence / structure	—	Lot / Batch	ZX261007-280 / B90958
Mol. formula	C39H56N12O10S	Manufacture date	7 Oct 2026
Mol. weight	908.03 g/mol	Date of analysis	9 Oct 2026
CAS number	2259213-56-8	Storage	-20 °C, dark, desiccated
Salt form	Acetate salt		

2. ANALYTICAL TEST RESULTS

Test	Method	Specification	Result	Verdict
Appearance	Visual	White/off-white powder	White to off-white lyophilized powder	PASS
Identity (ESI-MS)	LC-MS	Matches 908.03 Da	908.04 Da (Δ 11 ppm)	PASS
Purity	RP-HPLC, UV 220 nm	$\geq 98.0\%$ area	99.30%	PASS
Related substances	RP-HPLC	Single ≤ 1.0 / Total $\leq 2.0\%$	0.37 / 0.70%	PASS
Water content	Karl Fischer (USP <921>)	$\leq 8.0\%$	2.7%	PASS
Counter-ion: acetate	Ion chromatography	Report (3.0–15.0%)	5.0%	PASS
Net peptide content	Amino-acid analysis	$\geq 80.0\%$	90.1%	PASS
Bacterial endotoxin	LAL kinetic (USP <85>)	< 5.0 EU/mg	0.06 EU/mg	PASS
Heavy metals	ICP-MS (ICH Q3D)	Conforms	Conforms	PASS

CONCLUSION

All tested parameters CONFORM to the acceptance specifications. The batch is of high chromatographic purity ($\geq 98\%$) with an impurity profile, identity and residual/contaminant results meeting pharmaceutical-grade quality requirements. Material released. Supporting RP-HPLC chromatogram and ESI-MS spectrum are appended on page 2.

DLW.

Dr. Li Wenhua

Analyst · 9 Oct 2026 · Zhongxi Research Institute

DGT.

Dr. Guo Tao (QC Manager)

Approved by · 9 Oct 2026 · Zhongxi Research Institute




APPENDIX — ANALYTICAL RAW DATA

N-Acetyl Semax Amidate 10mg · Lot ZX261007-280 · Cert. ZXR-COA-2026-73712




Scan to verify

Figure 1. RP-HPLC Chromatogram (UV 220 nm)

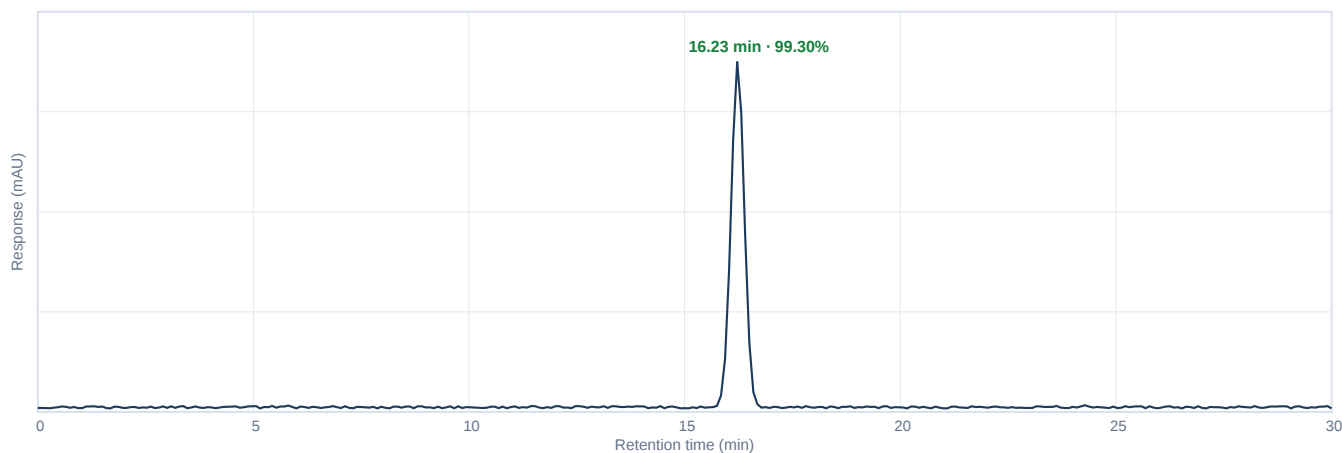

Peak #	RT (min)	Area (μV·s)	Area %	Assignment
1	16.23	1016913	99.30	Main (target)
2	5.68	3318	0.32	Impurity / related substance
3	24.27	2975	0.28	Impurity / related substance
4	23.74	1091	0.10	Impurity / related substance

Figure 2. ESI-MS Spectrum (positive ion mode)

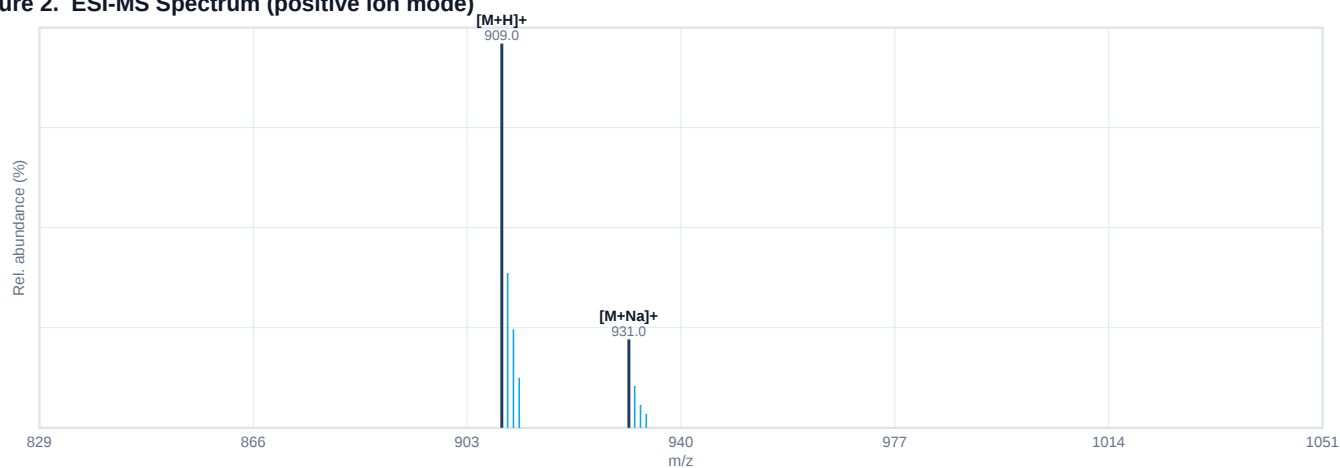

Interpretation

Identity confirmed by ESI-MS. Observed ions [M+H]⁺ 909.0, [M+Na]⁺ 931.0 deconvolute to a neutral monoisotopic-average mass of 908.04 Da (theoretical 908.03 Da; mass error 11 ppm), consistent with N-Acetyl Semax Amidate. No co-eluting species above 0.5% indicative of misidentification.

Methods — RP-HPLC: Agilent 1260 Infinity II; Zorbax SB-C18 4.6×250 mm, 5 μm; A: 0.1% TFA in water, B: 0.1% TFA in MeCN; 10–70% B over 30 min; 1.0 mL/min; 25 °C; 20 μL injection. MS: AB Sciex TripleTOF, ESI+, capillary 4.5 kV, deconvolution by Bio Tool Kit. KF: Metrohm 901. IC: Thermo Dionex ICS-6000. ICP-MS: Agilent 7900.